


# Restraint Minimisation

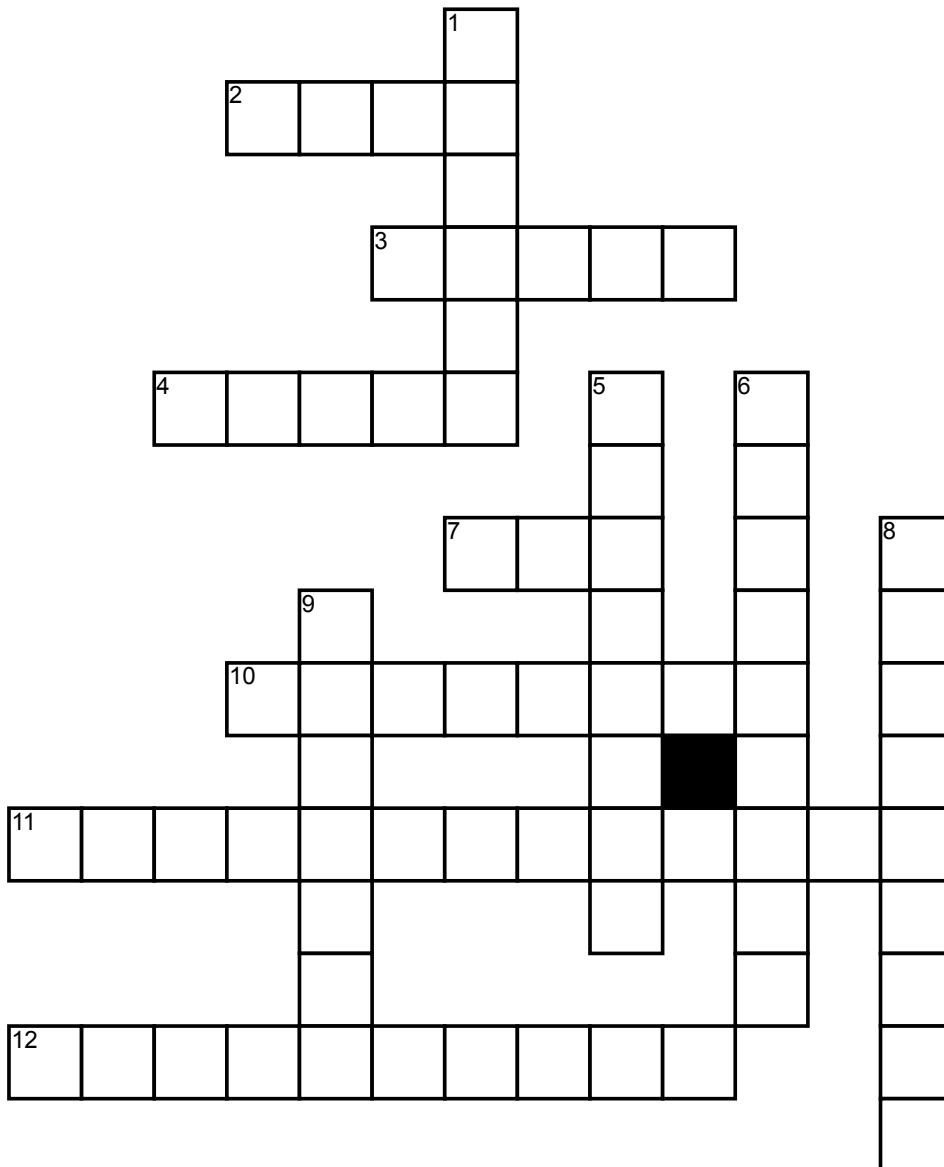

**Across**

- 2. A patient watch monitoring record is to be completed for \_\_\_\_\_ shift.
- 3. Where restraint or enabler is used, the \_\_\_\_\_ restrictive practices are used.
- 4. Both enablers and restraints \_\_\_\_\_ the normal freedom of the patient.
- 7. During de-escalation only \_\_\_\_\_ person should communicate with the person being de-escalated.

- 10. \_\_\_\_\_ Are not considered a form of restraint if used for patient safety during transportation and put down as soon as destination is reached.
  - 11. Restraint use is discontinued when there is no longer \_\_\_\_\_ to continue use.
  - 12. Restraint shall be clinically justified, safe and based on appropriate patient \_\_\_\_\_.
- Down**
- 1. Restraint shall not be used for the purpose of \_\_\_\_\_ to achieve compliance.

- 5. Medications used to render the person incapable of resistance are a form of \_\_\_\_\_ restraint, which is in breach of NZS8134.2:2008.
- 6. The use of restraint will be discussed with the patient on \_\_\_\_\_.
- 8. The use of an enabler shall be \_\_\_\_\_ and intended to promote independence, comfort and safety of patient.
- 9. The use of restraint is a \_\_\_\_\_ intervention that requires a clinical decision and rationale