


Sterile Processing

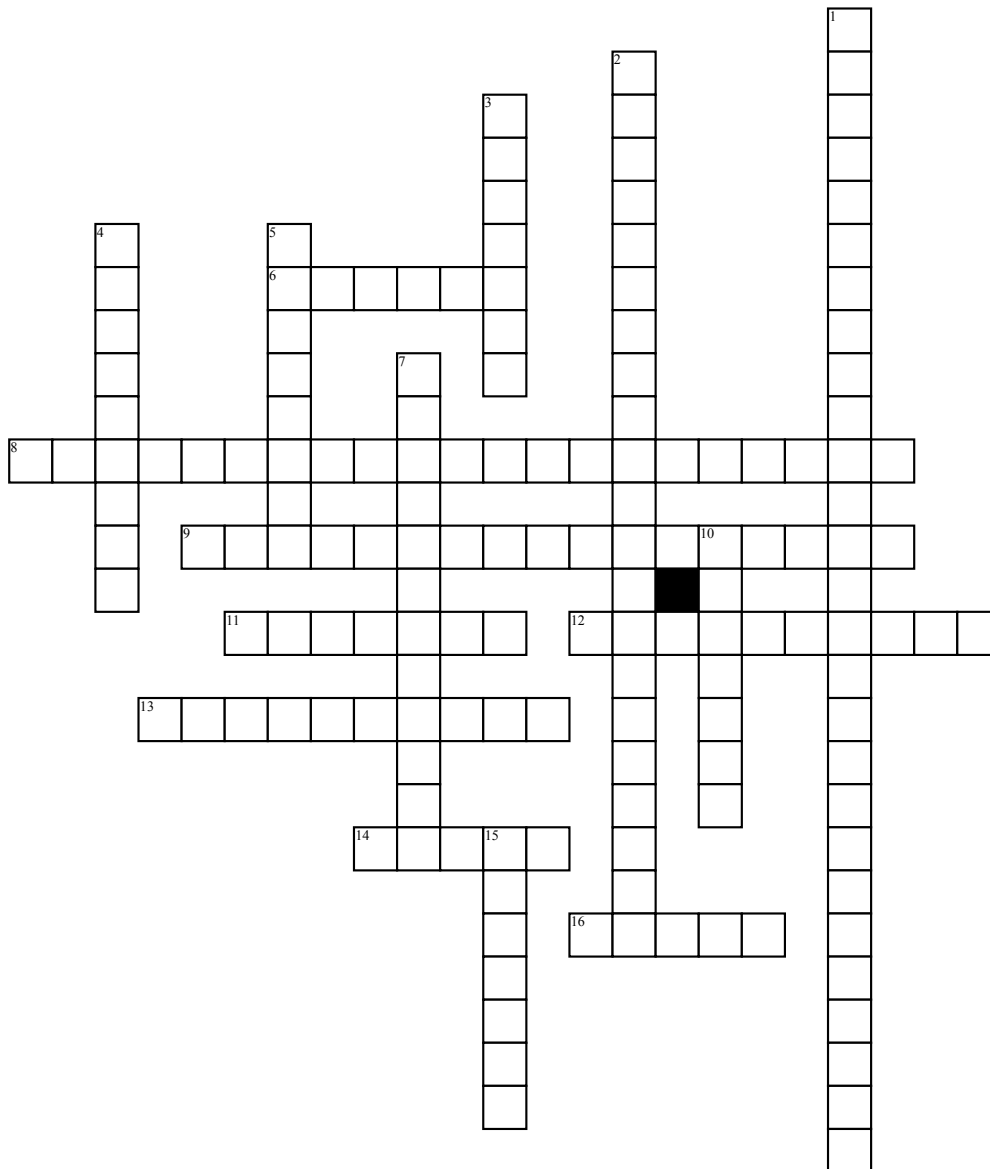

Across

6. item used to discern a stain from rust on an instrument

8. low temperature sterilization

9. used to recall instruments in a load

11. bubbles that form on instruments during the sonic process do this to clean

12. process where items are viewed closely for detail

13. test to ensure lethality of a sterilization load

14. special pouch used for hydrogen peroxide

16. process type most frequently used to sterilize items

Down

1. items used during instrument decontamination

2. kills most organisms except spores

3. an unprocessed biological

4. test performed daily in prevacuum sterilizers

5. must be performed on all endoscopes prior to cleaning

7. instrument flow

10. items intentionally retained during surgery

15. breaks down proteins and fats