


Sterile Processing

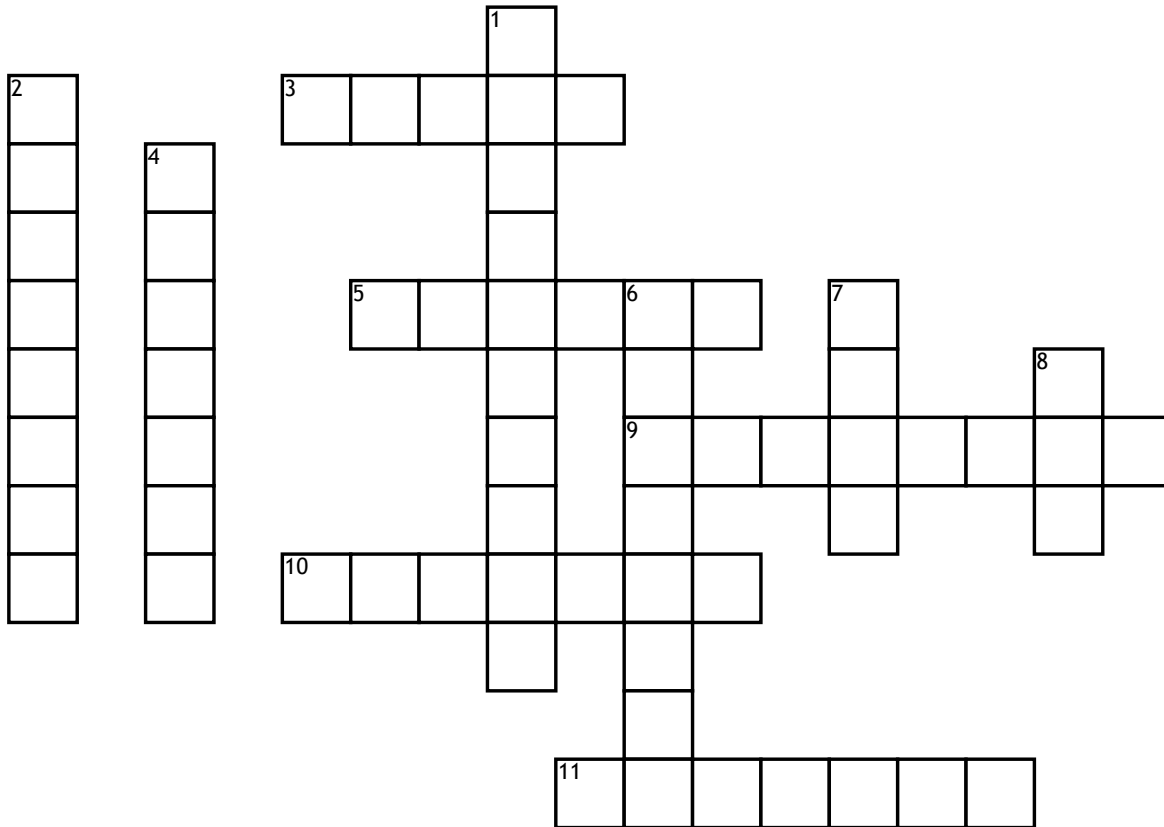

Across

3. this item must be tilted for drainage, so if water is present, it will run out
5. microorganisms capable of creating a thick wall
9. capable causing disease
10. At the end of the exposure phase, the chamber's drain is opened and the steam is removed through the discharge line.
11. package or containers with moisture after the sterilization process is completed

Down

1. which indicators are the most important sterilizer monitor
2. what devices cannot be released before the BI results are known
4. consistent delivery of products and services according to established standards
6. After the desired temperature is reached, the sterilizer's control system begins timing the cycle's exposure phase
7. concerned with safe work environment and employee safety
8. what color test material for 4.5 or larger instrument